


NEW Helix CT ICP Spray Chamber

Consistent day-to-day analytical performance is just a click away with ConstantTorque technology.

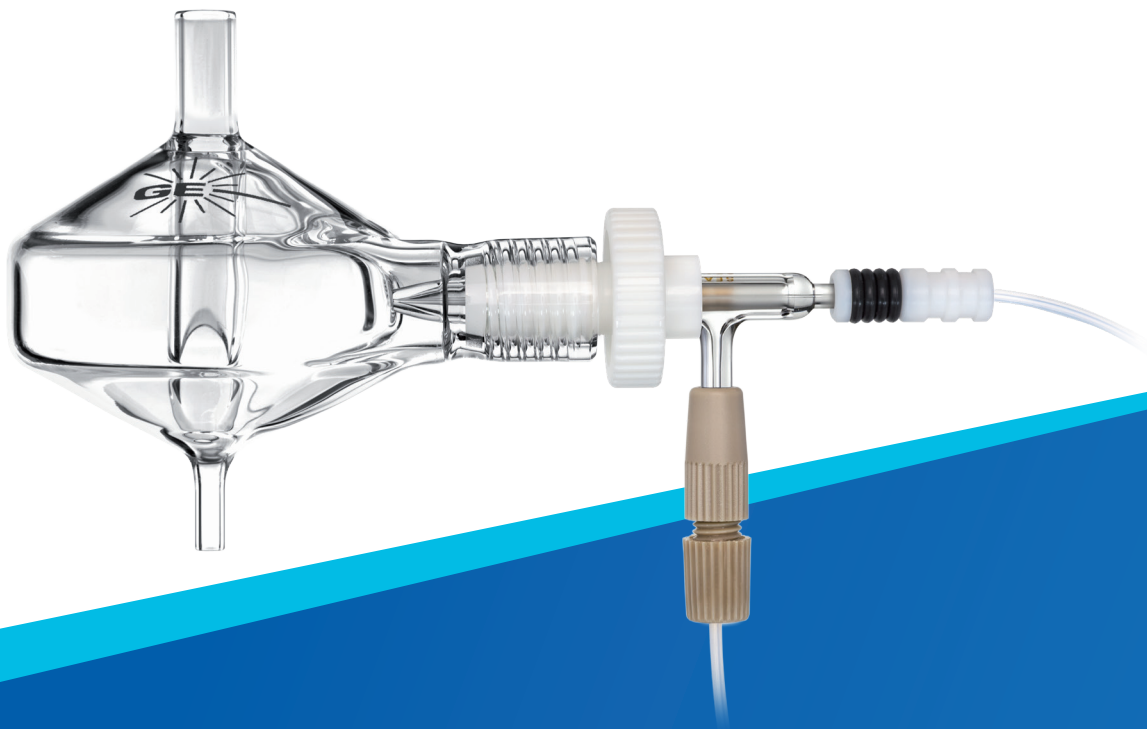

Glass Expansion now equips all of its glass, PFA, and PTFE spray chambers with the Helix CT (ConstantTorque) nebulizer interface to provide an optimum seal between the nebulizer and spray chamber.

Learn more at: www.geicp.com/HelixCT



GLASS EXPANSION
Quality By Design

International

6 Central Boulevard, Port Melbourne,
Vic 3207, Australia
Telephone: +61 3 9320 1111 Toll Free
(Aust): 1800 777 638
Facsimile: +61 3 9320 1112 Email:
enquiries@geicp.com

Americas

4 Barlows Landing Road Unit 2A,
Pocasset, MA 02559, USA
Telephone: 508 563 1800
Toll Free (US): 800 208 0097
Facsimile: 508 563 1802 Email:
geusa@geicp.com

Benefits of the New Helix CT Design Include...


ConstantTorque™ Locking Screw

A new Helix locking screw with CT technology allows for a consistent inert PTFE seal against the nebulizer - making it impossible to overtighten while ensuring a gas-tight seal each and every time. Torque control also improves user safety, preventing broken glassware.



PTFE PressFit™ Seal


A new PressFit Helix PTFE seal provides a chemically inert seal around the nebulizer. The PTFE ferrule is immune to strong acids and organic solvents routinely used in ICP sample preparation. It therefore eliminates all the drawbacks of the O-ring nebulizer seal, including broken nebulizers.

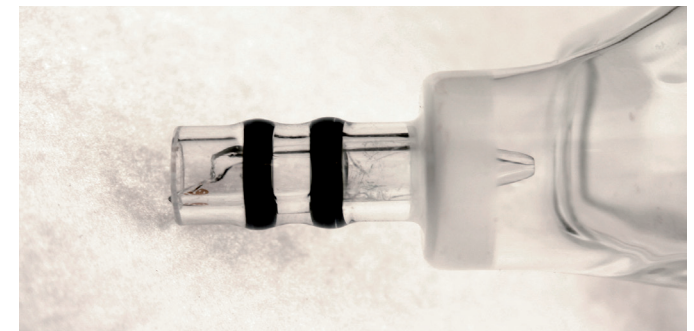

Prevents Nebulizer Bonding and Breaking

Zero Dead Volume Interface

Compared to other types of nebulizer-spray chamber interfaces, the Helix CT is the only interface that significantly reduces dead volume around the nebulizer. This unique design minimizes washout time with highly concentrated samples, reduces sample to sample carry-over and improves sample throughput.

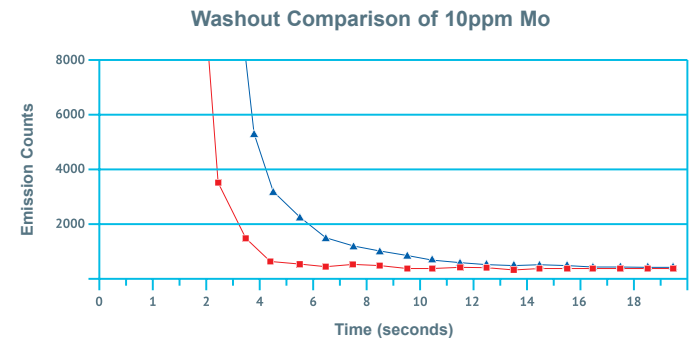

■ Helix Interface

▲ Non-Helix Interface

Optimum Depth and Torque

The new Helix CT interface still maintains the original positive stop to ensure that the nebulizer is inserted to the correct and optimum depth within the spray chamber. However, the torque applied to the nebulizer seal is also critical. Consistent nebulizer depth combined with ConstantTorque provides the ICP analyst with unparalleled, reproducible day-to-day analytical performance.

